



Lowest compliance
in class¹ avoiding
dog-bone effect

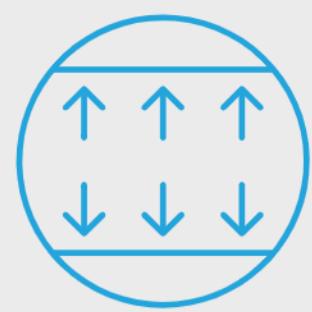

Precise
dilatation²

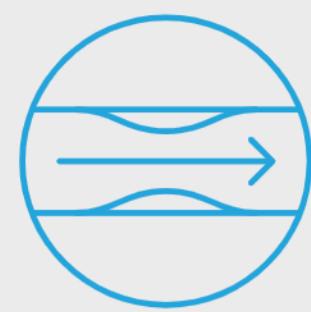

Enhanced
crossability²



Technical data/
ordering info


Teleflex[™]

Empowering the future of healthcare

Pantera[™] LEO

Non-Compliant High Pressure Balloon Catheter

Lowest compliance in class, precise dilatation
and enhanced crossability

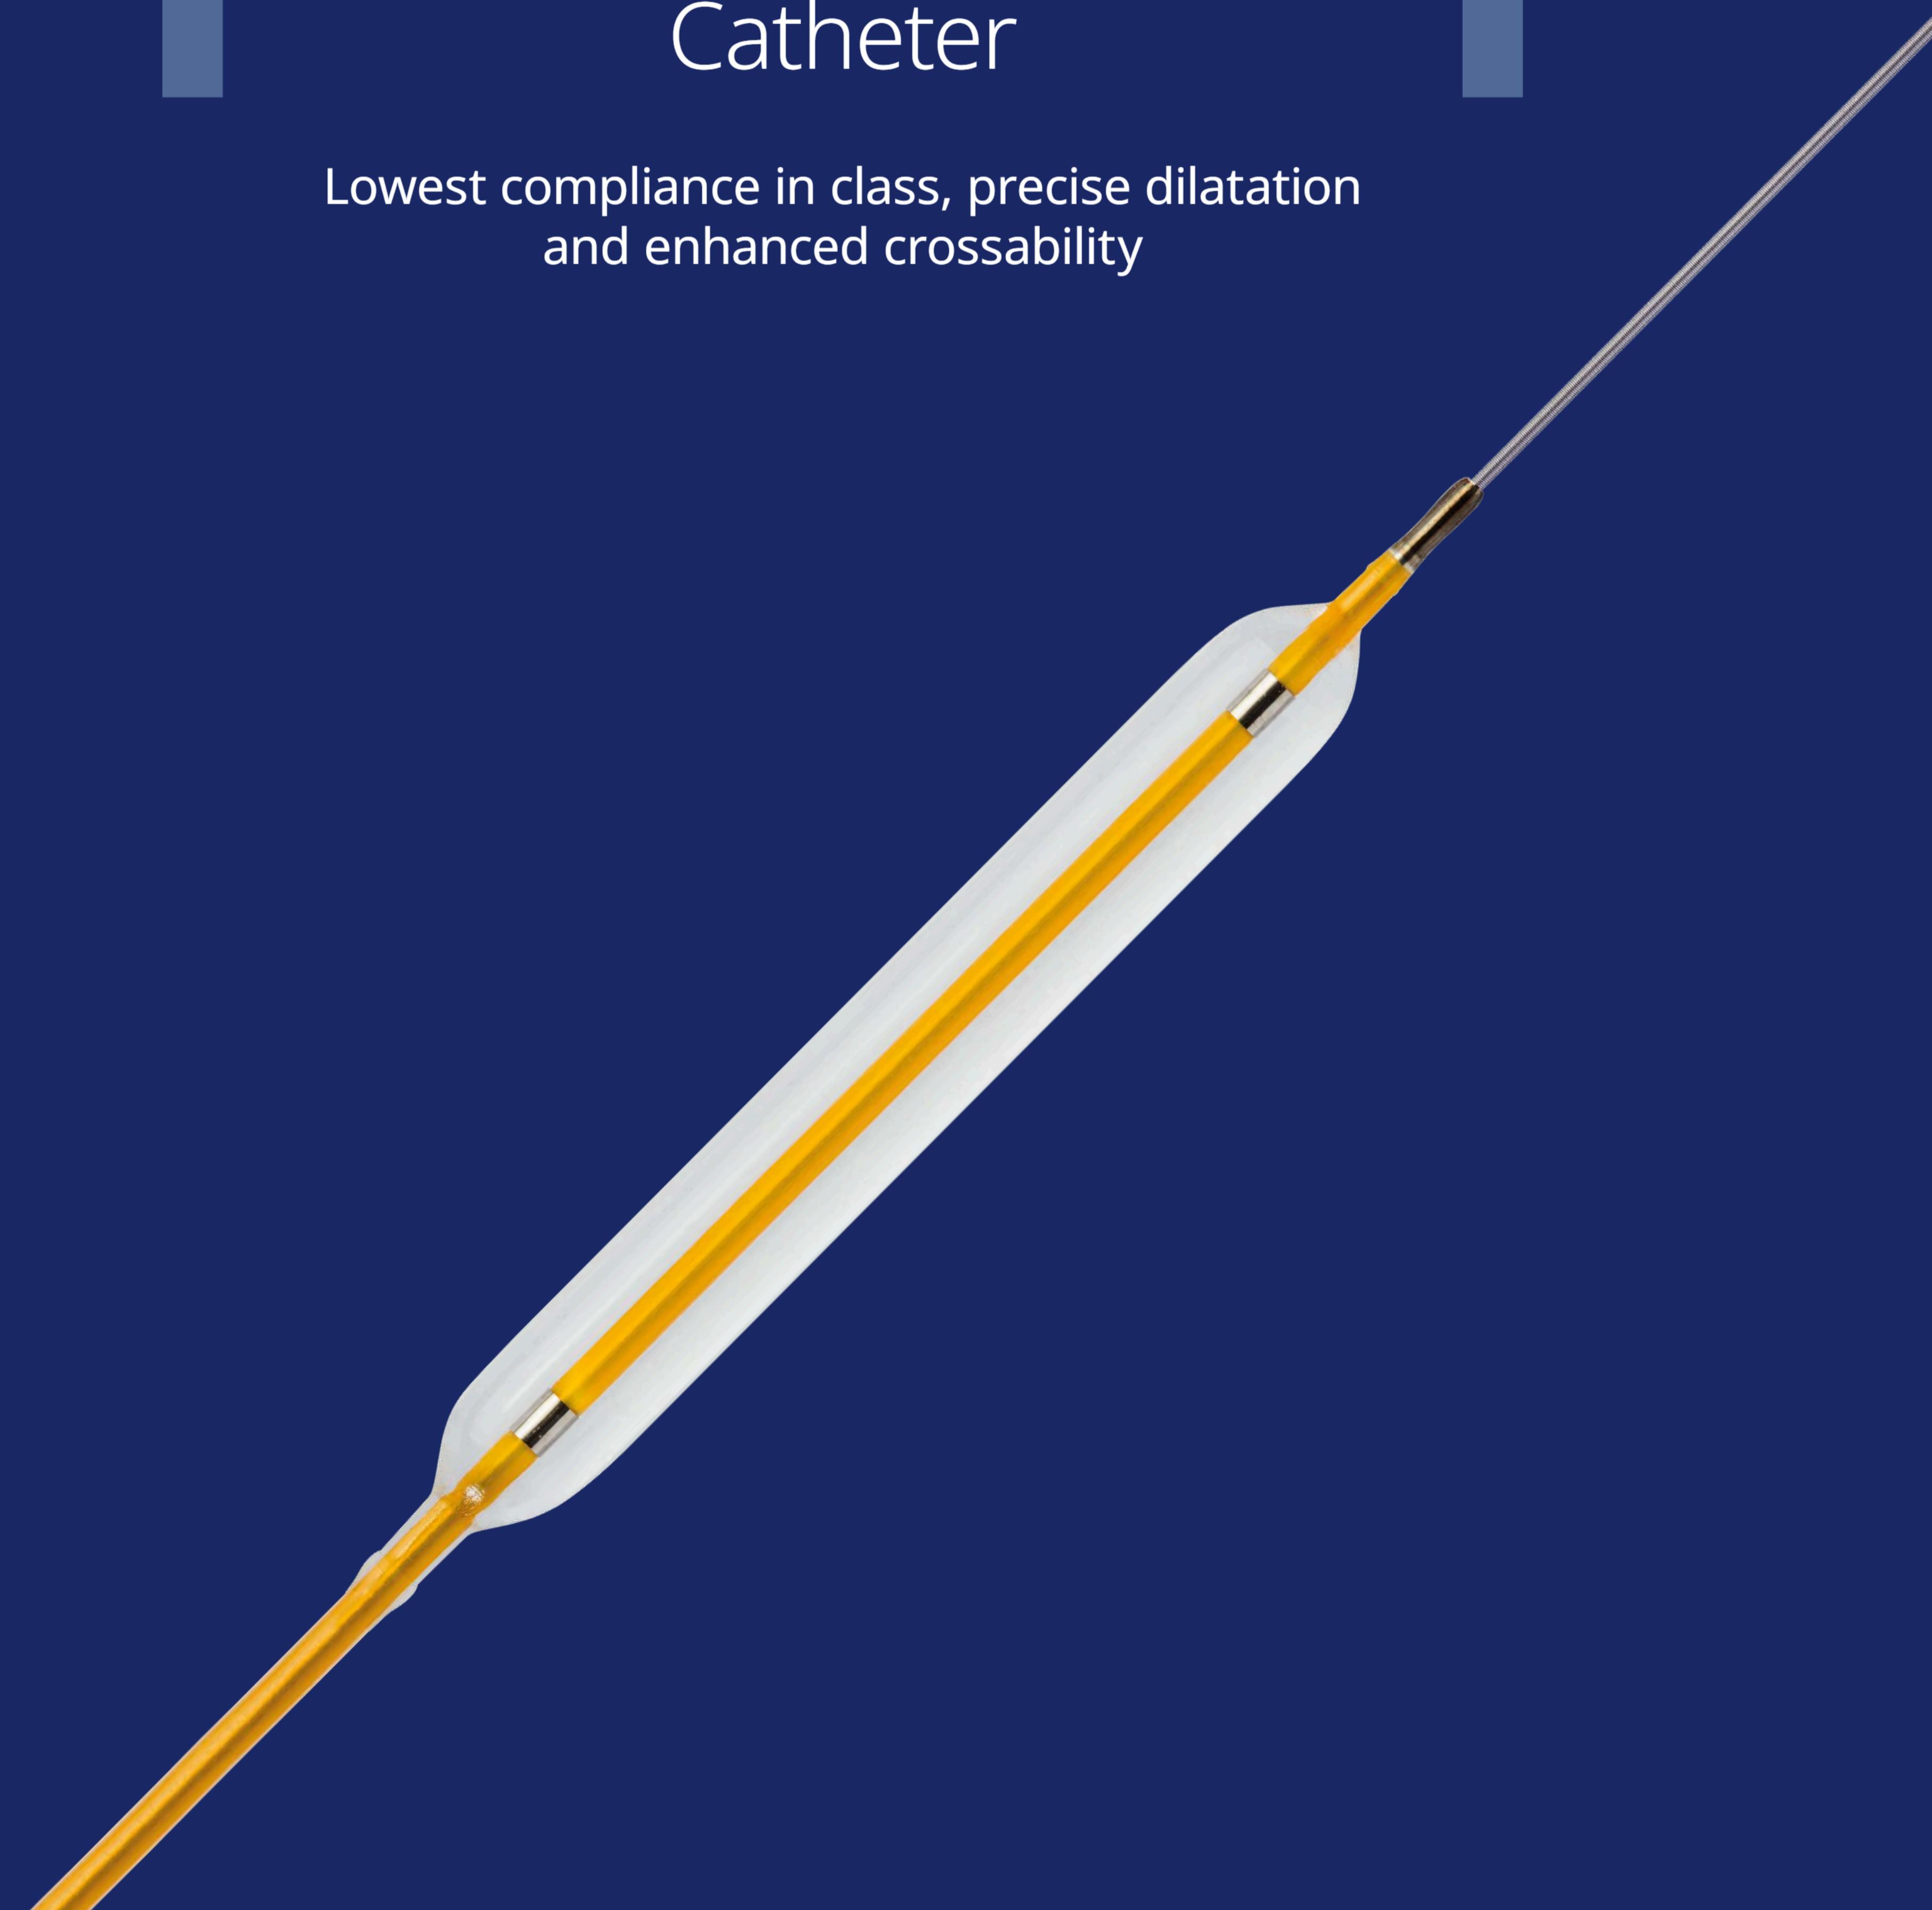

Pantera™ LEO


Lowest compliance in class, precise dilatation and enhanced crossability.

Lowest compliance in class¹ avoiding dog-bone effect

The Pantera™ LEO high pressure balloon has the lowest compliance in class¹ which ensures controlled minimal growth up to Rated Burst Pressure (RBP) without any dog-bone effect.

More controlled growth from Nominal Pressure (NP) to RBP¹

Compliance curves 3.0 mm balloons (Values shown between NP and RBP)

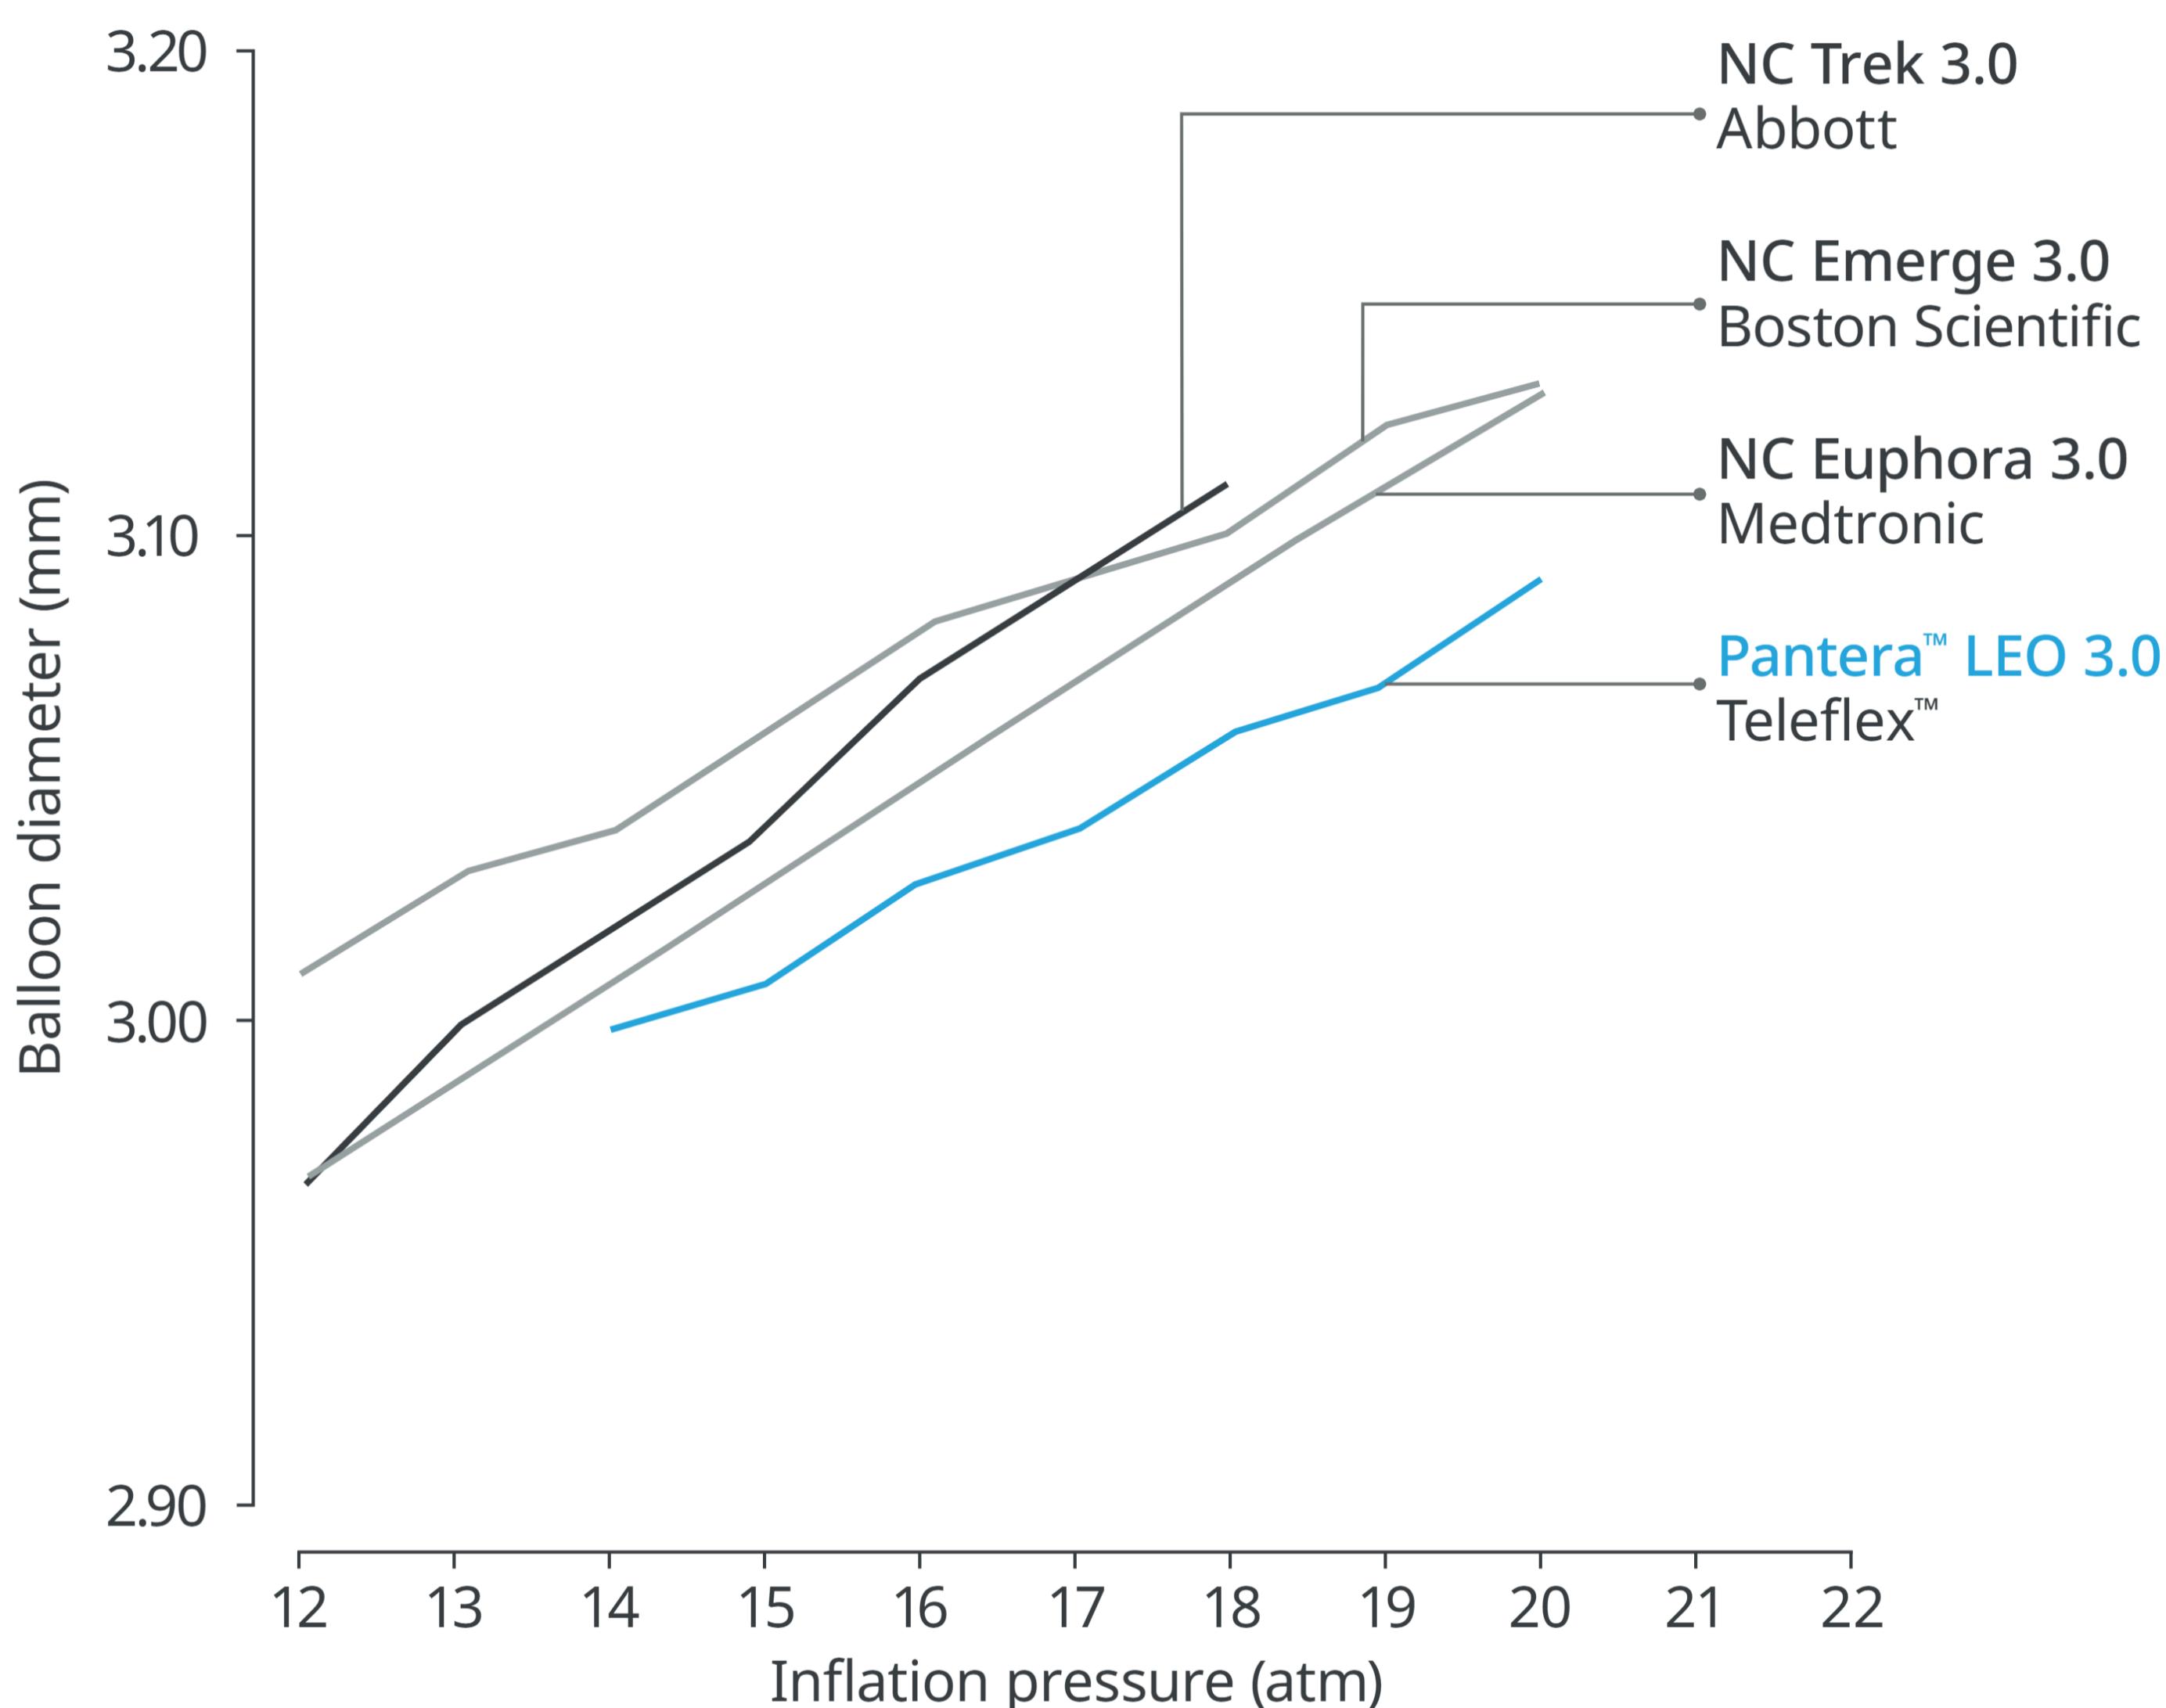



Precise dilatation²

Extra short balloon shoulders

The extra short balloon shoulders reduce longitudinal balloon growth, minimizing the potential for vessel trauma outside the treatment area.


Longitudinal balloon growth between NP and RBP²

Pantera™ LEO
Teleflex™

NP at 14 atm


Extra short shoulders

Minimal growth

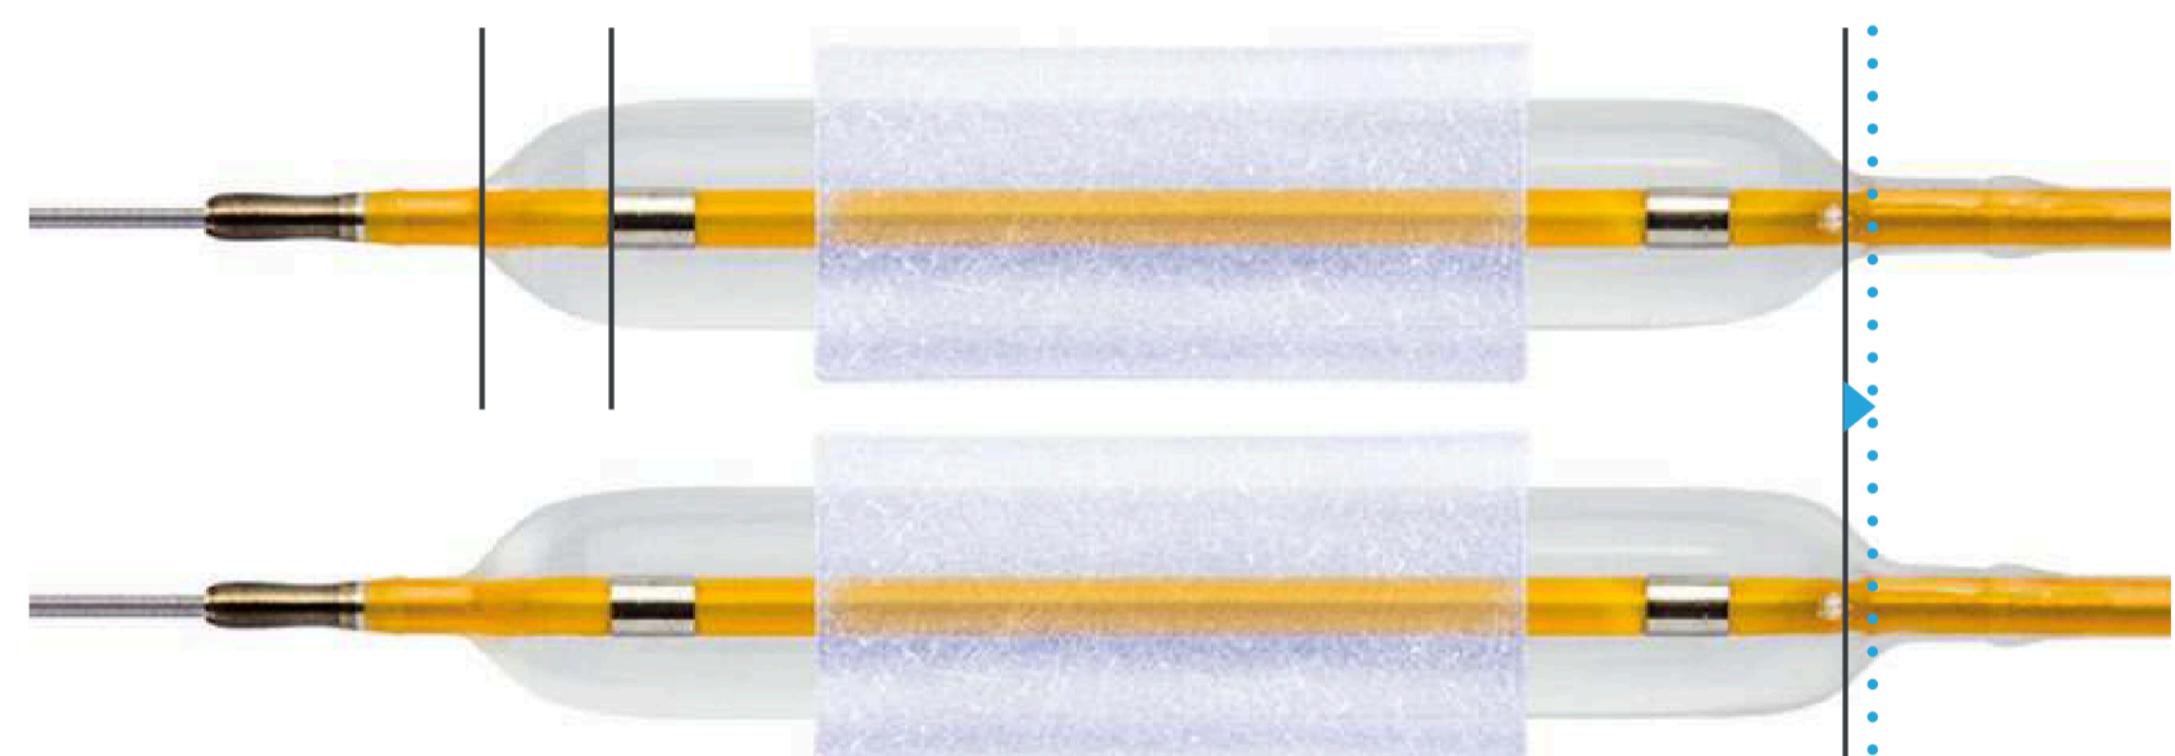

NC Emerge
Boston Scientific


NP at 12 atm

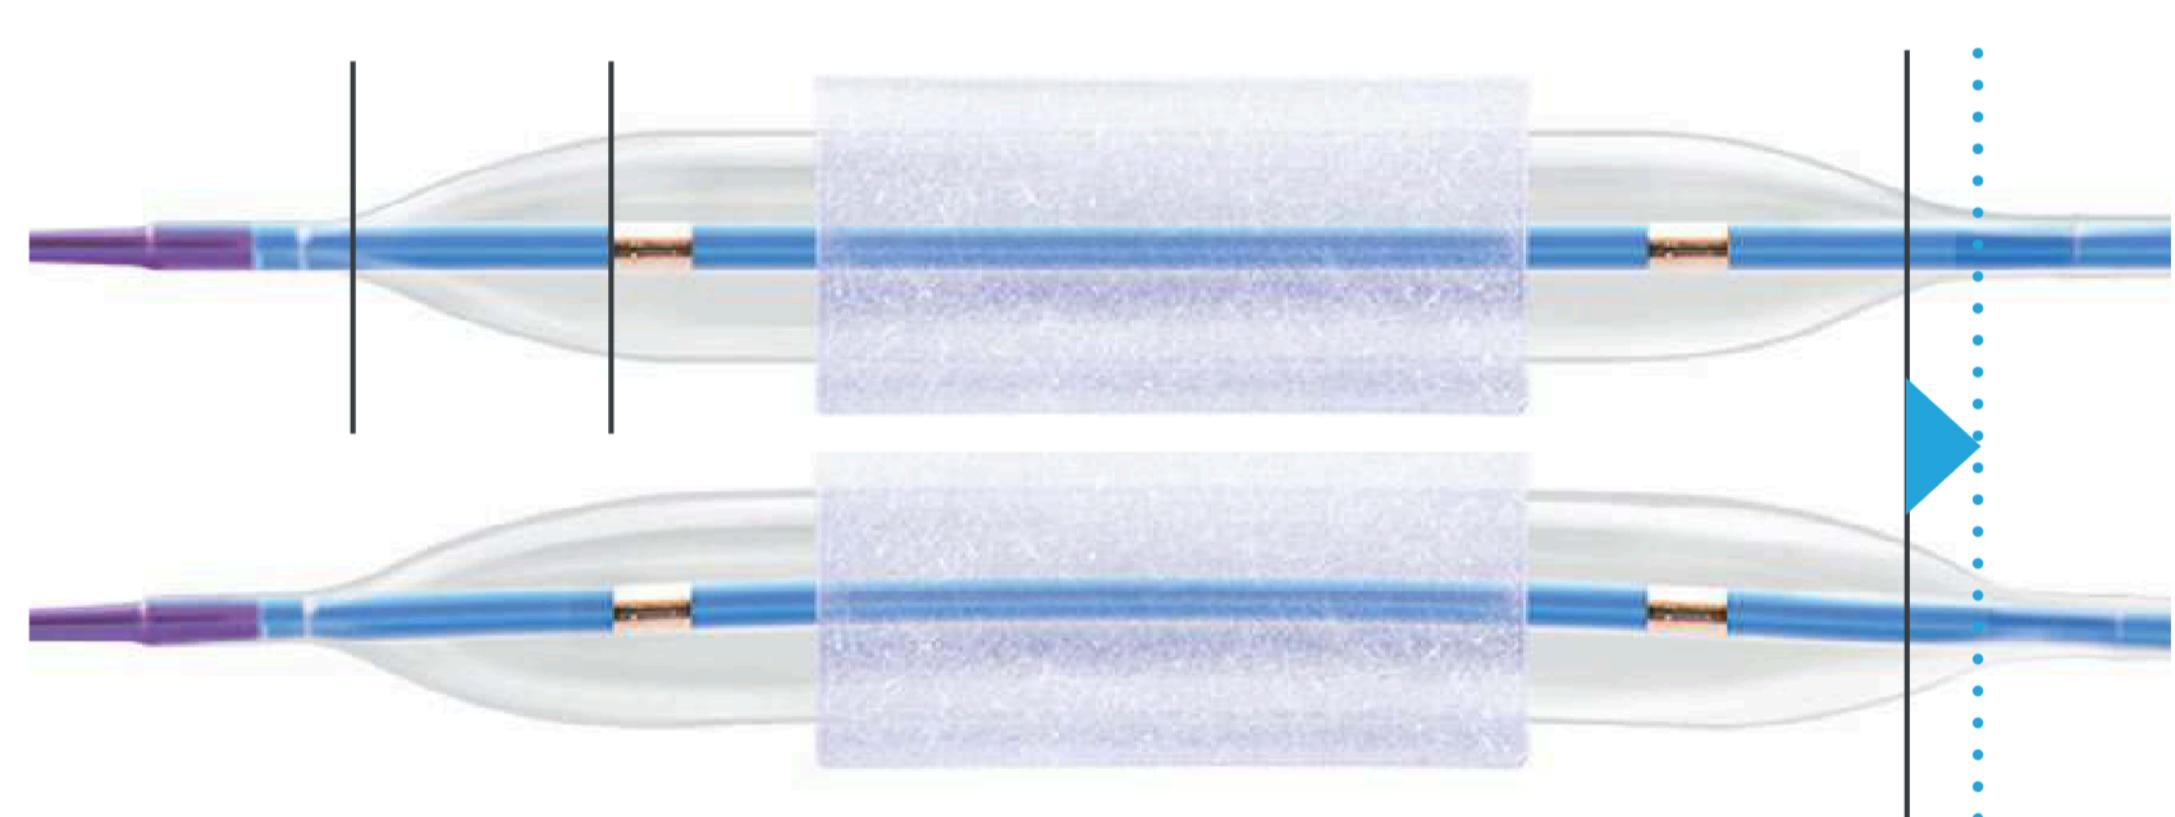

RBP at 20 atm

0 10 mm



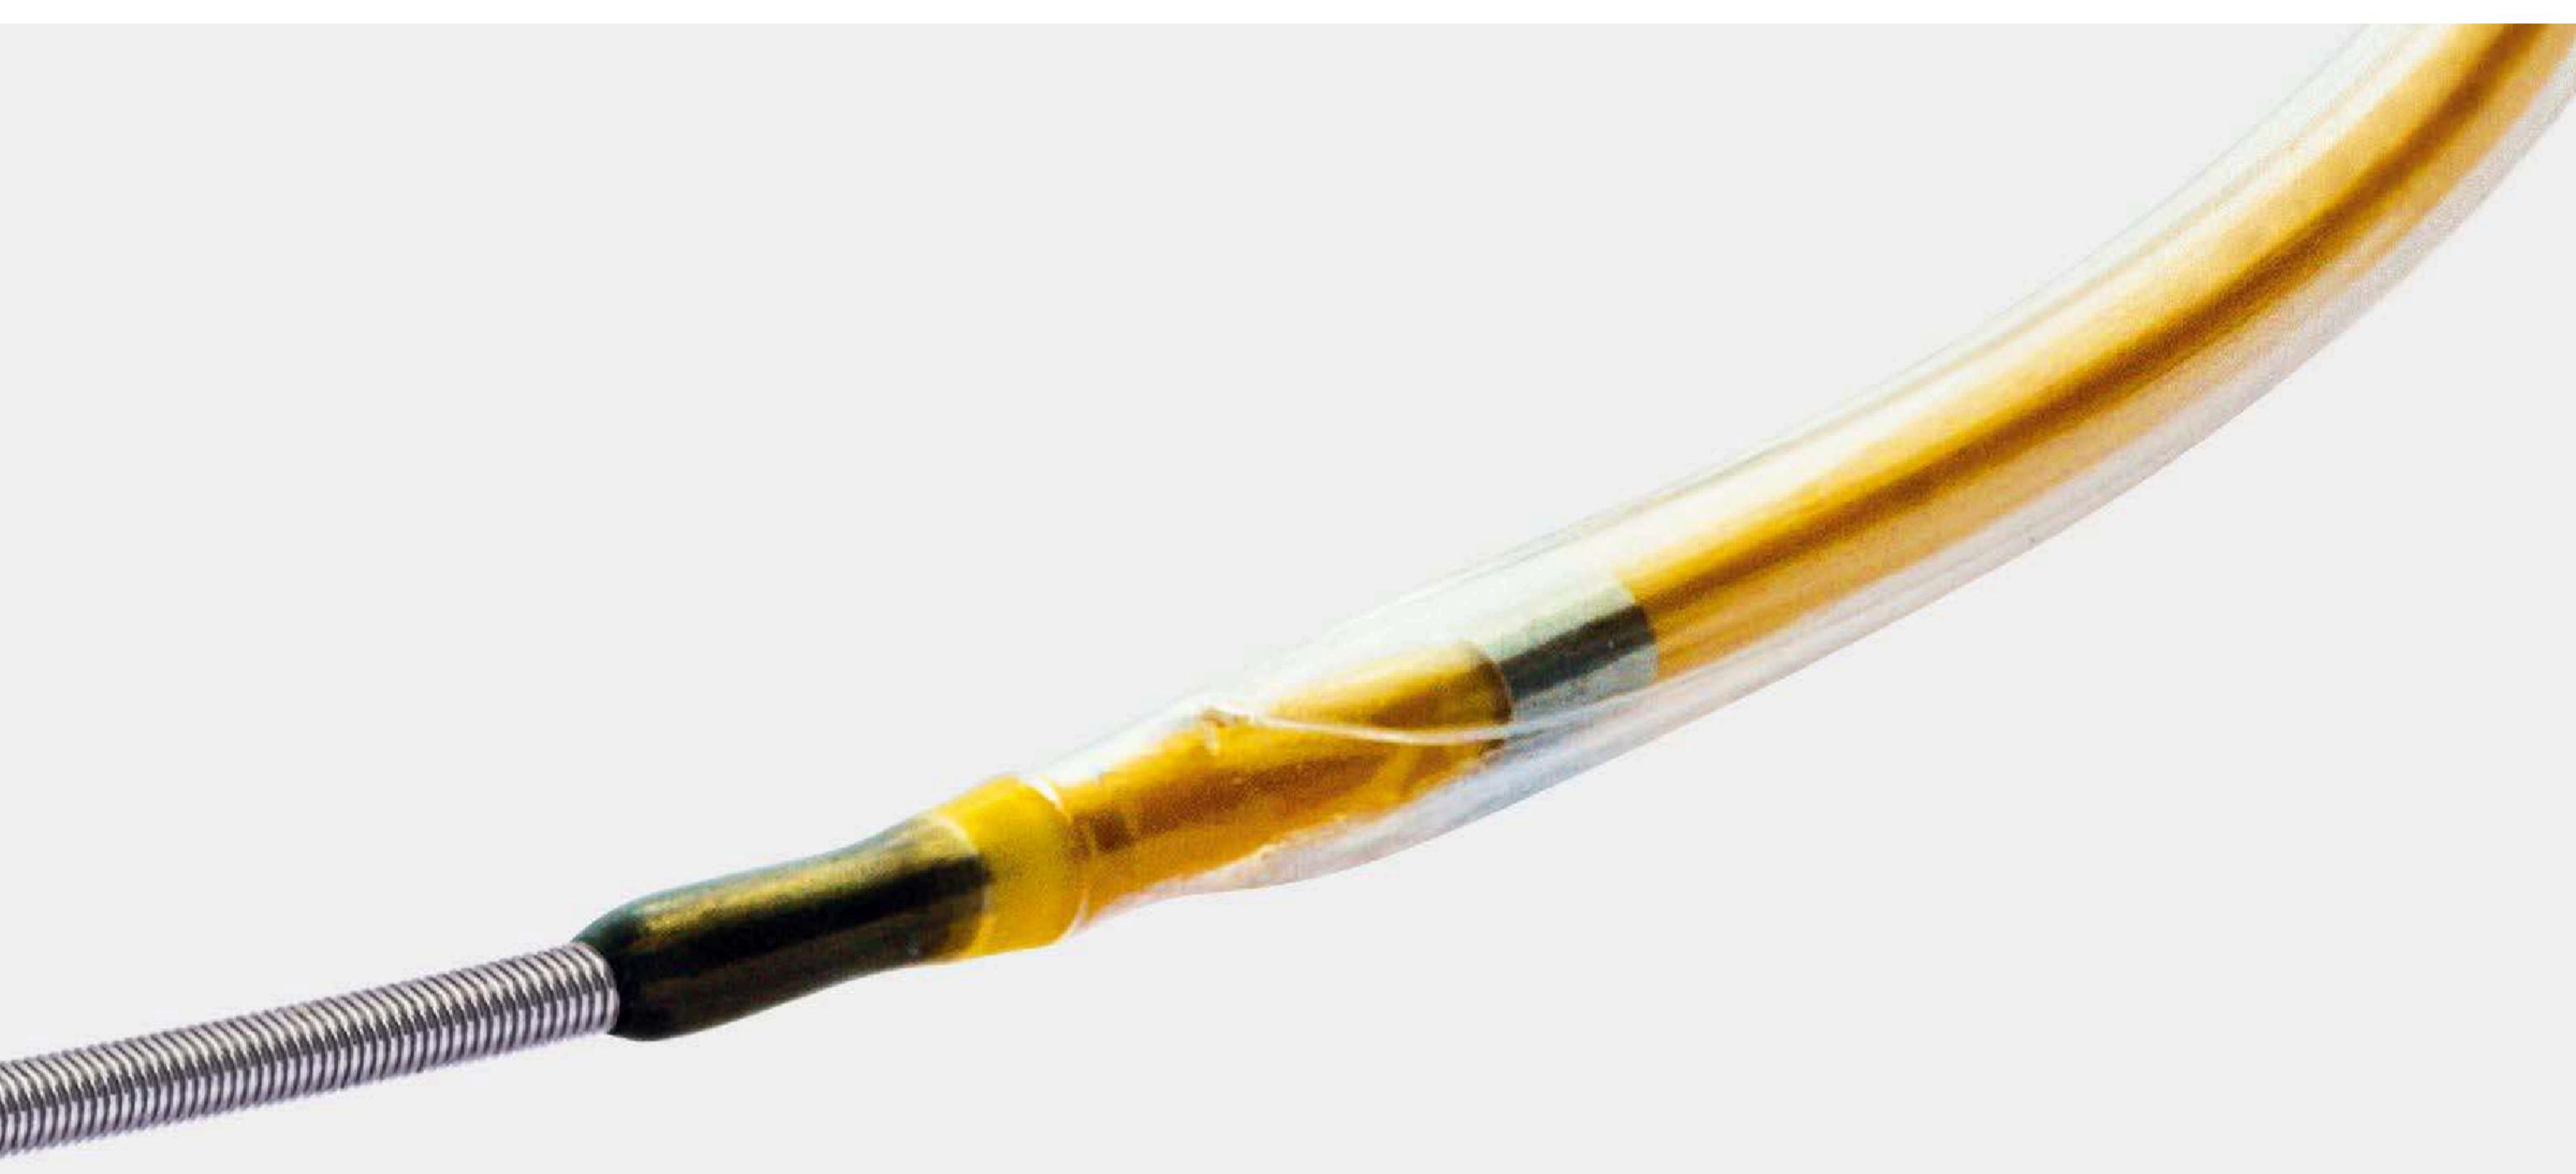


Enhanced crossability²

Patchwork coating


The tri-fold balloon is fully coated when folded but only partially coated when inflated. The resulting patchwork coating enables enhanced crossability while minimizing slippage during dilatation.




Folded balloon

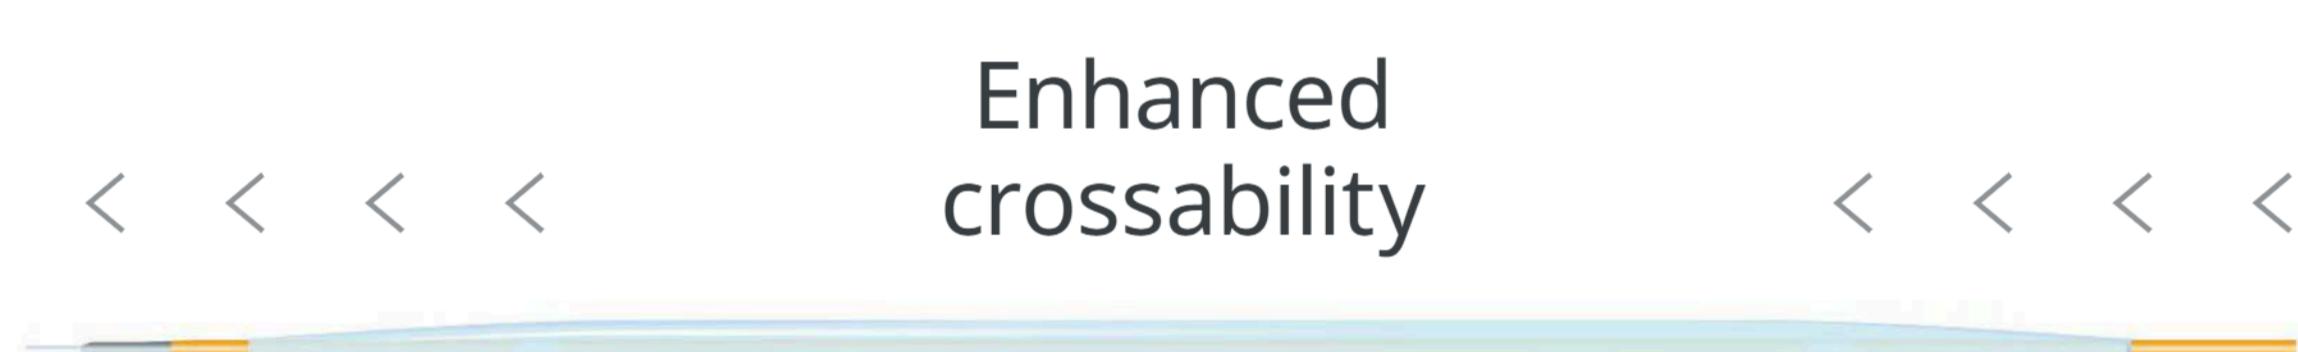

Enhanced crossability

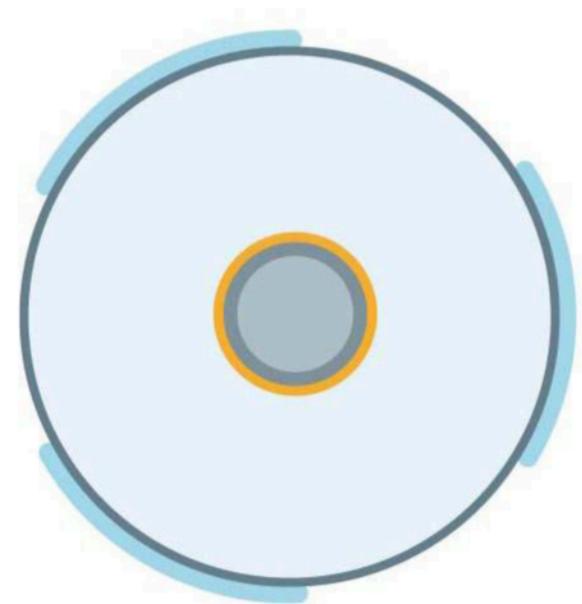

Inflated balloon

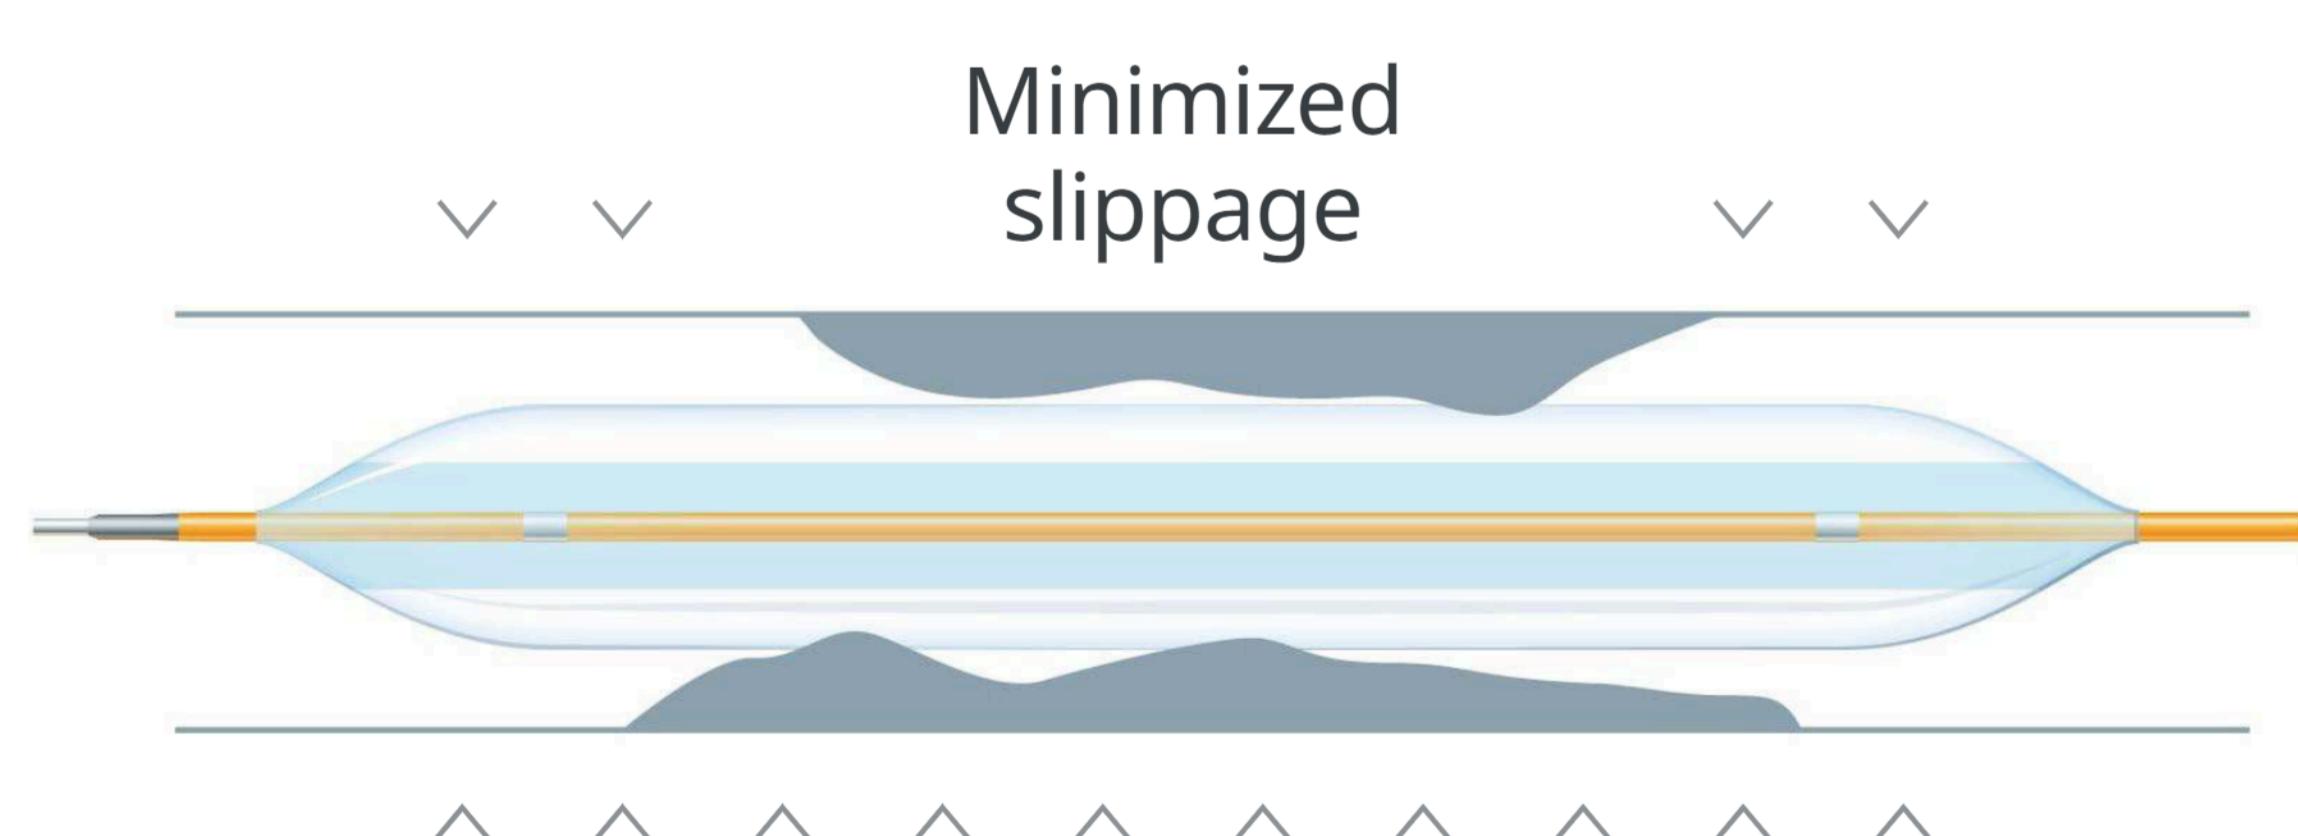

Minimized slippage



● Hydrophobic coating

○ Uncoated



Pantera™ LEO

Indicated for stent post-dilatation and dilatation of a coronary artery or bypass graft stenosis.*

Vascular
Intervention
Coronary



Technical data

PROXIMAL SHAFT	
Design	Hypotube design
Diameter	2.0F
Shaft markers	92 cm and 102 cm from tip
Coating	Hydrophobic
DISTAL SHAFT	
Guiding catheter	5F (min. I.D. 0.056")
Guide wire diameter	0.014"
Lesion entry profile	0.018"
Usable length	145 cm
Distal shaft length	34 cm
Balloon material	SCP (Semi Crystalline Polymer)
Balloon folding	3-fold
Balloon markers	Platinum-Iridium
Coating	Hydrophilic (end of balloon to guide wire exit port); hydrophobic (balloon and tip)
Diameter	2.6F (Ø 2.0–3.75 mm); 2.7F (Ø 4.0–5.0 mm)

Compliance Chart

		BALLOON DIAMETER × LENGTH (MM)											
		Ø 2.00 × 8-30	Ø 2.25 × 8-30	Ø 2.50 × 8-30	Ø 2.75 × 8-30	Ø 3.00 × 8-30	Ø 3.25 × 8-30	Ø 3.50 × 8-30	Ø 3.75 × 8-30	Ø 4.00 × 8-30	Ø 4.50 × 8-30	Ø 5.00 × 8-30	
Nominal Pressure (NP)	atm**	14	14	14	14	14	14	14	14	14	14	14	
	Ø (mm)	2.00	2.25	2.50	2.75	3.00	3.25	3.50	3.75	4.00	4.50	5.00	
Rated Burst Pressure (RBP)	atm**	20	20	20	20	20	20	20	20	20	18	18	
	Ø (mm)	2.05	2.32	2.57	2.83	3.09	3.35	3.61	3.89	4.12	4.56	5.07	

**1 atm = 1.013 bar

Ordering Information

BALLOON Ø	CATHETER LENGTH 145 CM, BALLOON LENGTH					
	8 mm	12 mm	15 mm	20 mm	30 mm	
2.00 mm	366991	367002	367013	367024	367035	
2.25 mm	366992	367003	367014	367025	367036	
2.50 mm	366993	367004	367015	367026	367037	
2.75 mm	366994	367005	367016	367027	367038	
3.00 mm	366995	367006	367017	367028	367039	
3.25 mm	366996	367007	367018	367029	367040	
3.50 mm	366997	367008	367019	367030	367041	
3.75 mm	366998	367009	367020	367031	367042	
4.00 mm	366999	367010	367021	367032	367043	
4.50 mm	367000	367011	367022	367033	367044	
5.00 mm	367001	367012	367023	367034	367045	

*Indication as per IFU.

References:

- 1 When compared to main competitors, compliance curves 3.0 mm balloons, data on file.
- 2 Data on file.

Teleflex, the Teleflex logo, and Pantera are trademarks or registered trademarks of Teleflex Incorporated or its affiliates in the U.S. and/or other countries. All other names are the trademarks or registered trademarks of their respective owners. Information in this material is not a substitute for the product Instructions for Use. Not all products may be available in all countries. Please contact your local representative.

© 2025 Teleflex Incorporated. All rights reserved.

369835-EN · REV H · 09 25 PDF · DV

Distributed by:

Teleflex Headquarters International, Ireland · Teleflex Medical Europe Ltd. · IDA Business & Technology Park
Dublin Road · Athlone · Co Westmeath · Tel. +353 (0)9 06 46 08 00 · Fax +353 (0)14 37 07 73 · orders.intl@teleflex.com

United Kingdom Tel. +44 (0)14 94 53 27 61 · info.uk@teleflex.com

South Africa Tel. +27 (0)11 807 4887 · assist.africa@teleflex.com

teleflex.com

Teleflex™
Empowering the future of healthcare